


HI733

Ammonia High Range

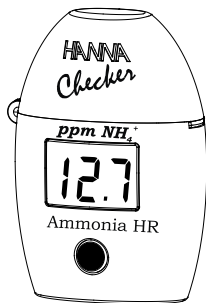

HANNA
instruments

www.hannainst.com

Dear Customer,

Thank you for choosing a Hanna Instruments Product.

Please read this instruction manual carefully before using the instrument. If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com or view our worldwide contact list at www.hannainst.com.

Preliminary examination

Please examine this product carefully. Make sure that the instrument is not damaged. If any damage occurred during shipment, please contact your local Hanna Instruments Office. Each HI733 meter is supplied complete with:

- Sample Cuvettes and Caps (2 pcs.)
- One bottle of Reagent A
- One bottle of Reagent B
- 1.5V AAA Battery (1 pc.)
- Instruction Manual and Quick Reference Guide




For more details about spare parts and accessories see "Accessories".

Technical specifications

Range	0.0 to 99.9 ppm as NH_4^+
Resolution	0.1 ppm
Accuracy	± 1.0 ppm $\pm 5\%$ of reading @ 25 °C / 77 °F
Light Source	Light Emitting Diode @470 nm
Light Detector	Silicon Photocell
Method	Adaptation of the ASTM Manual of Water and Environmental Technology, D1426-92, Nessler method. The reaction between ammonia and reagents causes a yellow tint in the sample.
Environment	0 to 50 °C (32 to 122 °F); max 95% RH non-condensing
Battery Type	1.5V AAA (1 pc.)
Auto-Shut off	After 10 minutes of non-use
Dimensions	86.0 x 61.0 x 37.5 mm (3.4 x 2.4 x 1.5")
Weight	52 g (1.84 oz.)

Functional description



1. Dust cover.
2. Cuvette with cap.
3. Cuvette holder.
4. Liquid Crystal Display.
5. Button.

Errors and warnings

L.H.

Light High: There is too much light to perform a measurement. Please check the preparation of the zero cuvette.

L.Lo

Light Low: There is not enough light to perform a measurement. Please check the preparation of the zero cuvette.

Inu

Inverted Cuvettes: The sample and the zero cuvette are inverted.

0.0

Under Range: A blinking "0.0" indicates that the sample absorbs less light than the zero reference. Check the procedure and make sure you use the same cuvette for reference (zero) and measurement.

99.9

Over Range: A flashing value of the maximum concentration indicates the reading is over range. Dilute the sample and re-run the test.

bAt

Battery Low: The battery must be replaced soon.


bAd

Dead Battery: This indicates that the battery is dead and must be replaced. Once this indication is displayed, normal operation of the instrument will be interrupted. Change the battery and restart the meter.

bAt

Measurement procedure

- Turn the meter on by pressing the button. All segments will be displayed. When the display shows "Add", "C.1" with "Press" blinking, the meter is ready.
- Use the syringe to add 1 mL of unreacted sample to the cuvette. Add 9 mL of HI733B-0 reagent B to the cuvette, using the plastic pipette. Place the cap and swirl the solution to mix. Place the cuvette into the meter and close the meter's cap.
- Press the button. When the display shows "Add", "C.2" with "Press" blinking the meter is zeroed.
- Remove the cuvette from the meter and unscrew the cap. Add 4 drops of HI733A-0 reagent A. Replace the cap and swirl the solution. Place the cuvette back into the meter.
- Press and hold the button until the timer is displayed on the LCD (the display will show the countdown prior to the measurement) or, alternatively, wait for 3 minutes and 30 seconds and press the button.
- The instrument displays the results in mg/L (ppm) of ammonium ion (NH_4^+). To convert the reading to ppm of ammonia (NH_3), multiply the reading by the factor 0.944. To convert the reading to ppm of ammonia nitrogen ($\text{NH}_3\text{-N}$), multiply the reading by the factor 0.776. The meter automatically turns off after 10 minutes.

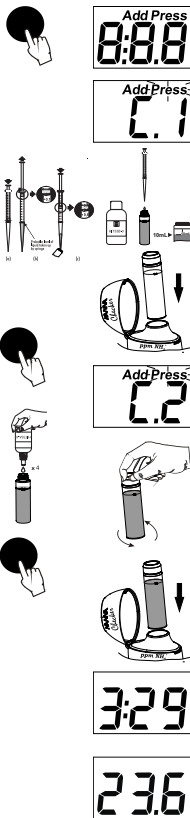

Tips for an accurate measurement

- It is important that the sample does not contain any debris.
- Whenever the cuvette is placed into the measurement cell, it must be dry outside, and completely free of fingerprints, oil and dirt. Wipe it thoroughly with HI731318 or a lint-free cloth prior to insertion.
- Shaking the cuvette can generate bubbles, causing higher readings. To obtain accurate measurements, remove bubbles by swirling or by gently tapping the cuvette.
- Do not let the reacted sample stand for too long after reagent is added, as accuracy will be affected.
- After the reading it is important to immediately discard the sample, otherwise the glass might become permanently stained.


Battery management

To save the battery, the instrument shuts down after 10 minutes of non-use. One fresh battery lasts for a minimum of 5000 measurements. When the battery is dead the instrument will display "bAd" then "bAt" for 1 second and then turns off.

To restart the instrument, the battery must be replaced with a new one.

To replace the instrument's battery:

- Turn the instrument off by holding the button until the meter shuts off.
- Turn the instrument upside down and remove the battery cover with a screwdriver.



- Remove the battery from its location and replace it with a new one, inserting the negative end first.
- Insert the battery cover and replace the screw with a screwdriver.

Recommendations for Users

Before using this product, make sure that it is entirely suitable for your specific application and for the environment in which it is used.

Operation of this instrument may cause unacceptable interferences to other electronic equipment, thus requiring the operator to take all necessary steps to correct interferences.

Any variation introduced by the user to the supplied equipment may degrade the instrument's EMC performance.

To avoid damage or burns, do not put the instrument in microwave oven. For the safety of you and the instrument do not use or store the instrument in hazardous environments.

Accessories

REAGENT SETS

HI733-25 Reagent set for 25 Ammonia High Range tests

OTHER ACCESSORIES

HI733-11 Ammonia HR Certified Standard Kit
HI731225 Cuvette Black Cap for Checker® HC Colorimeters (4 pcs.)
HI731318 Cloth for wiping cuvettes (4 pcs.)
HI731321 Glass Cuvettes and Seal Cap for Checker® HC Colorimeters (4 pcs.)
HI731353 Cuvette seal cap for checker HC (4 pcs.)
HI740028P 1.5V AAA batteries (12 pcs.)
HI740142P 1 mL graduated syringe (10 pcs.)
HI740144P Pipette tip (10 pcs.)
HI740157P Plastic refilling pipette (20 pcs.)
HI93703-50 Cuvette cleaning solution (230 mL)

Warranty

HI733 is warranted for a period of one year after date of purchase against defects in workmanship and materials when used for their intended purpose and maintained according to instructions. This warranty is limited to repair or replacement free of charge. Damage due to accidents, misuse, tampering or lack of prescribed maintenance is not covered. If service is required, contact your local Hanna Instruments Office. If under warranty, report the model number, date of purchase, serial number and the nature of the problem. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the instrument is to be returned to Hanna Instruments, first obtain a Return Goods Authorization number from the Technical Service department and then send it with shipping costs prepaid. When shipping any instrument, make sure it is properly packed for complete protection.

Hanna Instruments reserves the right to modify the design, construction or appearance of its products without advance notice.