


HI784

Marine Ammonia (NH₃/NH₄⁺)

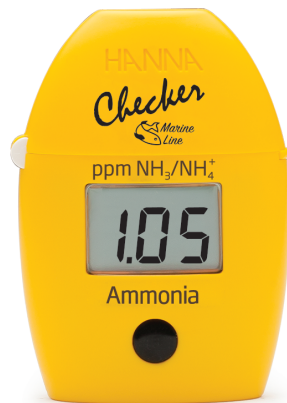

Disposal of waste batteries. This product contains batteries, do not dispose of them with other household waste. Hand them over to the appropriate collection point for recycling.

Ensuring proper product and battery disposal prevents potential negative consequences for the environment and human health. For more information, contact your city, your local household waste disposal service, or the place of purchase.

Recommendations for Users

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any variation introduced by the user to the supplied equipment may degrade the checker's performance. For your and the checker's safety do not use or store it in hazardous environments.

Warranty

HI784 Checker HC is warranted for a period of one year against defects in workmanship and materials when used for its intended purpose and maintained according to instructions. This warranty is limited to repair or replacement free of charge. Damage due to accidents, misuse, tampering, or lack of prescribed maintenance is not covered. If service is required, contact your local Hanna Instruments® office. If under warranty, report the model number, date of purchase, serial number, and the nature of the problem. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the checker is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization (RGA) number from the Technical Service department and then send it with shipping costs prepaid. When shipping any product, make sure it is properly packaged for complete protection.

Hanna Instruments reserves the right to modify the design, construction, or appearance of its products without advance notice.

All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA.


IST784 03/22

Battery Replacement

To save the battery, the checker shuts down after 20 minutes of non-use and 10 minutes after reading. A fresh battery lasts for a minimum of 5000 measurements. When the battery is drained, the instrument displays "bAd" then "bAt", and turns off.

To replace the battery, follow the next steps:

1. Press and hold the ON/OFF button to turn the checker off.
2. Turn the instrument upside down and use a screwdriver to unfasten the screw and remove the battery cover.
3. Remove the old battery, replace it with a new 1.5V AAA battery, inserting the negative end first.
4. Replace the battery cover, fasten and tighten the screw.



Accessories

Reagent Sets

HI784-25 Reagents for 25 Marine Ammonia tests

Other Accessories

HI784-11 Marine Ammonia certified standard kit

HI731315 Glass cuvette and cap for Checker® HC colorimeters (2 pcs.)

HI731318 Cloth for wiping cuvettes (4 pcs.)

HI740028P 1.5V AAA battery set (12 pcs.)

HI740157P Transfer pipette (20 pcs.)

HI93703-50 Cuvette cleaning solution, 230 mL

Certification

All Hanna® instruments conform to the CE European Directives.

Disposal of Electrical & Electronic Equipment. The product should not be treated as household waste. Instead, hand it over to the appropriate collection point for the recycling of electrical and electronic equipment, which will conserve natural resources.





RoHS compliant



Tips for an Accurate Measurement

- Ensure the sample does not contain any debris.
- Hold dropper bottles completely vertically and squeeze slowly to ensure correct drop size.
- Whenever the cuvette is placed into the checker, it must be dry outside and free of fingerprints, oil and dirt.
- Wipe the cuvette thoroughly with HI731318 microfiber cleaning cloth or a lint-free cloth prior to insertion.
- Shaking the cuvette can generate bubbles, causing higher readings. To obtain accurate measurements, remove such bubbles by swirling or by gently tapping the cuvette.
- Do not let the reacted sample stand too long after reagent has been added, as accuracy will be affected.
- Discard the sample immediately after the reading has been taken or the glass might become permanently stained.
- Prepare sample cuvette immediately after collecting sample from tank. Ammonia is volatile and will dissipate if stored in a bottle before analysis, causing low measurements.
- If the prepared sample cuvette becomes cloudy the measurement will not be accurate. Prepare a new sample by adding an extra 1-2 drops of HI784A-0 Reagent A.



Calculating Unionized Toxic Ammonia

This method measures NH₃/NH₄⁺. To determine the toxic NH₃ portion, use the table to determine the percentage of toxic NH₃. Levels of toxic NH₃ greater than 0.01 ppm have a negative effect on fish. Multiply total ammonia (NH₃/NH₄⁺) by the percent unionized ammonia from the table to determine unionized toxic ammonia.

Example: pH 8.0, Temperature: 24 °C (75 °F), NH₃/NH₄⁺ 1.00 ppm
 Unionized toxic ammonia: 1.00 ppm x (5.0 ÷ 100) = 0.05 ppm

Percentage of Unionized Ammonia (NH₃)

pH	21 °C (70 °F)	24 °C (75 °F)	26 °C (79 °F)	29 °C (84 °F)
7.6	1.7	2.1	2.4	2.9
7.8	2.6	3.2	3.7	4.5
8.0	4.1	5.0	5.8	7.0
8.2	6.3	7.7	8.8	11
8.4	9.7	12	13	16
8.6	15	17	20	23
8.8	21	25	28	32

Dear Customer,

Thank you for choosing a Hanna Instruments® product. Please read this instruction manual carefully before using the Checker® HC handheld colorimeter. For more information about Hanna Instruments and our products, visit www.hannainst.com or e-mail us at sales@hannainst.com. For technical support, contact your local Hanna Instruments office or e-mail us at tech@hannainst.com.

Preliminary Examination

Remove the Checker HC handheld colorimeter and accessories from the packing material and examine it carefully. If you require any further information, please contact Hanna Instruments technical support team.

Each HI784 is delivered in a case with custom insert and is supplied with:

- Marine Ammonia reagent starter kit (reagents for 10 tests)
- Sample cuvette and cap (2 pcs.)
- Plastic refilling pipette (1 pc.)
- 1.5V AAA Alkaline battery (1 pc.)
- Instruction manual
- Quick-reference guide

Note: Save all packing material until you are sure that the Checker HC handheld colorimeter works correctly. Any damaged or defective item must be returned in its original packing material with the supplied accessories.

General Description & Intended Use

HI784 Marine Ammonia handheld checker is designed to determine the concentration of ammonia in saltwater aquariums and marine biology applications.

HI784 features a single-button operation system and is easy to use.


The large LCD is easy to read and the auto shut-off feature assures the battery will not be drained.

Specifications

Range	0.00 to 2.50 ppm (mg/L) NH ₃
Resolution	0.01 ppm (mg/L)
Accuracy	±0.05 ppm ±5% of reading @ 25 °C (77 °F)
Light source	Light Emitting Diode @ 610 nm
Light detector	Silicon photocell
Method	Adaptation of the Salicylate Method. The reaction between Ammonia and Ammonium and the reagent causes a blue-green tint in the sample.
Environment	0 to 50 °C (32 to 122 °F); max. 95% RH non-condensing Prepared sample cuvette (sample plus reagents) must be 18 to 29 °C (65 to 85 °F)*.
Battery type	1.5V AAA Alkaline
Auto shut-off	After 20 minutes of non-use and 10 minutes after reading
Dimensions	86.0 x 61.0 x 37.5 mm (3.4 x 2.4 x 1.5")
Weight	64 g (2.3 oz)

* Warm or cool prepared cuvettes if needed.

Functional Description & LCD Display

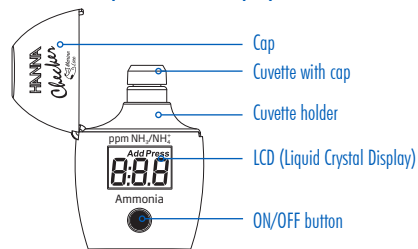

Measurement Procedure

1. Press the ON/OFF button to turn the checker on. All segments will be displayed for a few seconds, followed by "Add", "C.1" with "Press" blinking.

2. Preparing the cuvette for "C.1" measurements:

- Use the pipette to fill the cuvette with 10 mL of unreacted sample.
- Hold the HI784A-0 Reagent A dropper bottle vertically and add 18 drops to the cuvette.

Note: For best results, tap the dropper on a hard surface and clean the outside of the tip prior to use.

- Using scissors, open one packet of HI784B-0 Reagent B along the dotted line. Push the two corners together to make a spout. Add the content of the packet to the cuvette.

- Screw the cap onto the cuvette and invert until the powder is completely dissolved. Do NOT shake vigorously – this will cause more air bubbles!

For the most accurate reading, ensure all reagent is dissolved and there are no visible bubbles. Ensure the outside of the cuvette is dry and clean.

- Let the cuvette stand for 30 seconds. This allows complete dissipation of micro-bubbles.

- Insert the cuvette into the checker and close the cap.


- Press the ON/OFF button. When the display shows "Add", "C.2" with "Press" blinking, the checker is zeroed. Remove the cuvette.

3. Preparing the cuvette for "C.2" measurements:

- Unscrew the cuvette cap. Hold the HI784C-0 Reagent C dropper bottle vertically and add 12 drops to the cuvette.

- Replace the cap and invert the cuvette 5 times to mix.

- Insert the cuvette into the checker and close the cap.

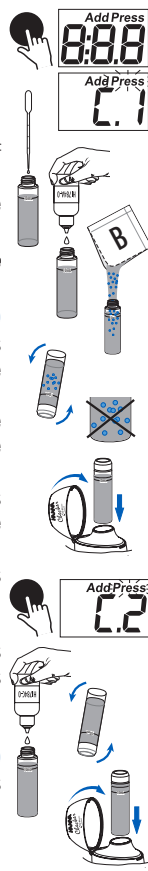

- Press and hold the ON/OFF button. The display will show the countdown prior to the measurement. Alternatively, wait 15 minutes and press the button once to measure.



Note: For samples with less than 1.00 ppm, the reaction is complete after 10 minutes. Users may press the ON/OFF button at this time, with 5 minutes remaining on the timer.

- When the timer ends, the checker will perform the reading. The instrument displays the ammonia/ammonium concentration in ppm NH₃. The checker automatically turns off 10 minutes after reading.
- To calculate the unionized ammonia (NH₃) concentration, use the conversion table on the reverse side.

Errors & Warnings

The checker shows clear warning messages when erroneous conditions appear and when measured values are outside the expected range. The information below provides an explanation of the errors and warnings, and the recommended action to be taken.

Light High: There is an excess amount of ambient light reaching the detector. Please check preparation of zero cuvette.

Light Low: There is not enough light to perform a measurement. Please check the preparation of the zero cuvette.

Under Range: Minimum concentration value displayed blinking indicates the measured value is outside the limits of the method. Verify that the sample does not contain any debris, and the preparation of the sample cuvette.

Over Range: Maximum concentration value displayed blinking indicates the measured value is outside the limits of the method. Verify the preparation of the sample cuvette. Dilute the sample and repeat the measurement.

Battery Low: Battery level is too low for the checker to function properly. Replace the battery with a new one.

Drained Battery: The battery is drained and must be replaced. Replace the battery with a new one and restart the checker.

L.H.

L.Lo

0.00

2.50

bAt

bAd

bAt